



10X6-1800 The Radiation Protection Chamber

For very low-level radiation measurements such as shielding, leakage, irradiators and environmental. Superior to typical survey meters for accuracy.

Specifications¹

Rate Specifications

0.1 mR/hr - 18 mR/s
0.1 µGy/hr - 200 µGy/s

Exposure Specifications

1 nR - 196 R
0.01 nGy - 1.7 Gy

Auto Dose Threshold

7 µR/s
63 pGy/s

Cine Specifications:

N/A

Calibration Accuracy:

±4% using X-rays @ 150 kVp & 10.2 mm Al HVL

Exposure Rate Dependence:

±0%, -5%, 0.1 mR/hr to 20 R/hr, -10% to 65 R/hr

Energy Dependence

±5%, 30 keV to 1.33 MeV

Construction:


Concentric cylinders. polycarbonate walls and electrode; conductive graphite exterior coating; 1800 cm³ active volume; 3.2 mm wall nominal; 0.54 kg

Environmental:


15° - 35° C working, 0° - 60° C storage, < 80% RH (non-condensing), 70-106 kPa

Minimum Field Size²:

177 mm x 140 mm

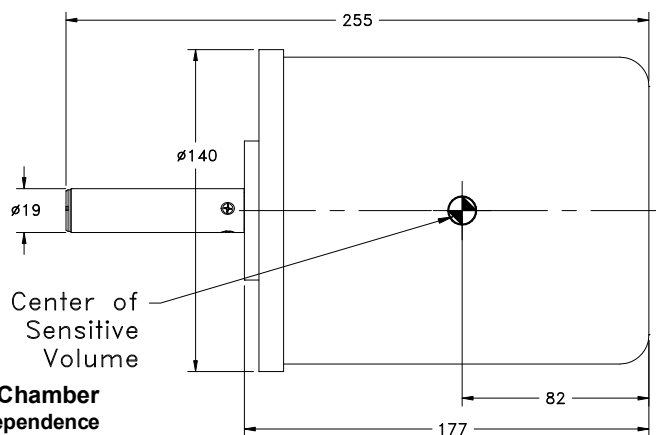

**-1800 Ion Chamber
Energy Dependence
(TYPICAL)**

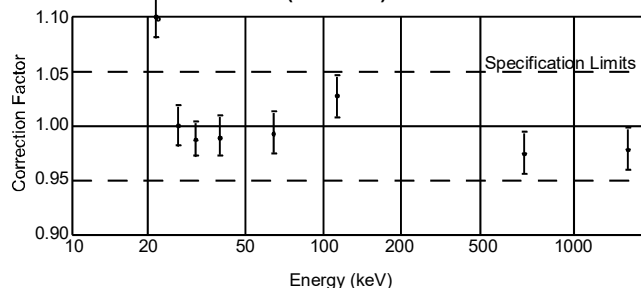

Dimensions in millimeters

Warning: Introduction of material other than air behind the chamber will cause its response to change due to backscatter.

¹Specifications apply when used with Accu-Gold series digitizer.

² A field size greater than the Minimum Field Size by at least 10 mm recommended.